

This Page Is Inserted by IFW Operations  
and is not a part of the Official Record

## BEST AVAILABLE IMAGES

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images may include (but are not limited to):

- BLACK BORDERS
- TEXT CUT OFF AT TOP, BOTTOM OR SIDES
- FADED TEXT
- ILLEGIBLE TEXT
- SKEWED/SLANTED IMAGES
- COLORED PHOTOS
- BLACK OR VERY BLACK AND WHITE DARK PHOTOS
- GRAY SCALE DOCUMENTS

**IMAGES ARE BEST AVAILABLE COPY.**

**As rescanning documents *will not* correct images,  
please do not report the images to the  
Image Problem Mailbox.**

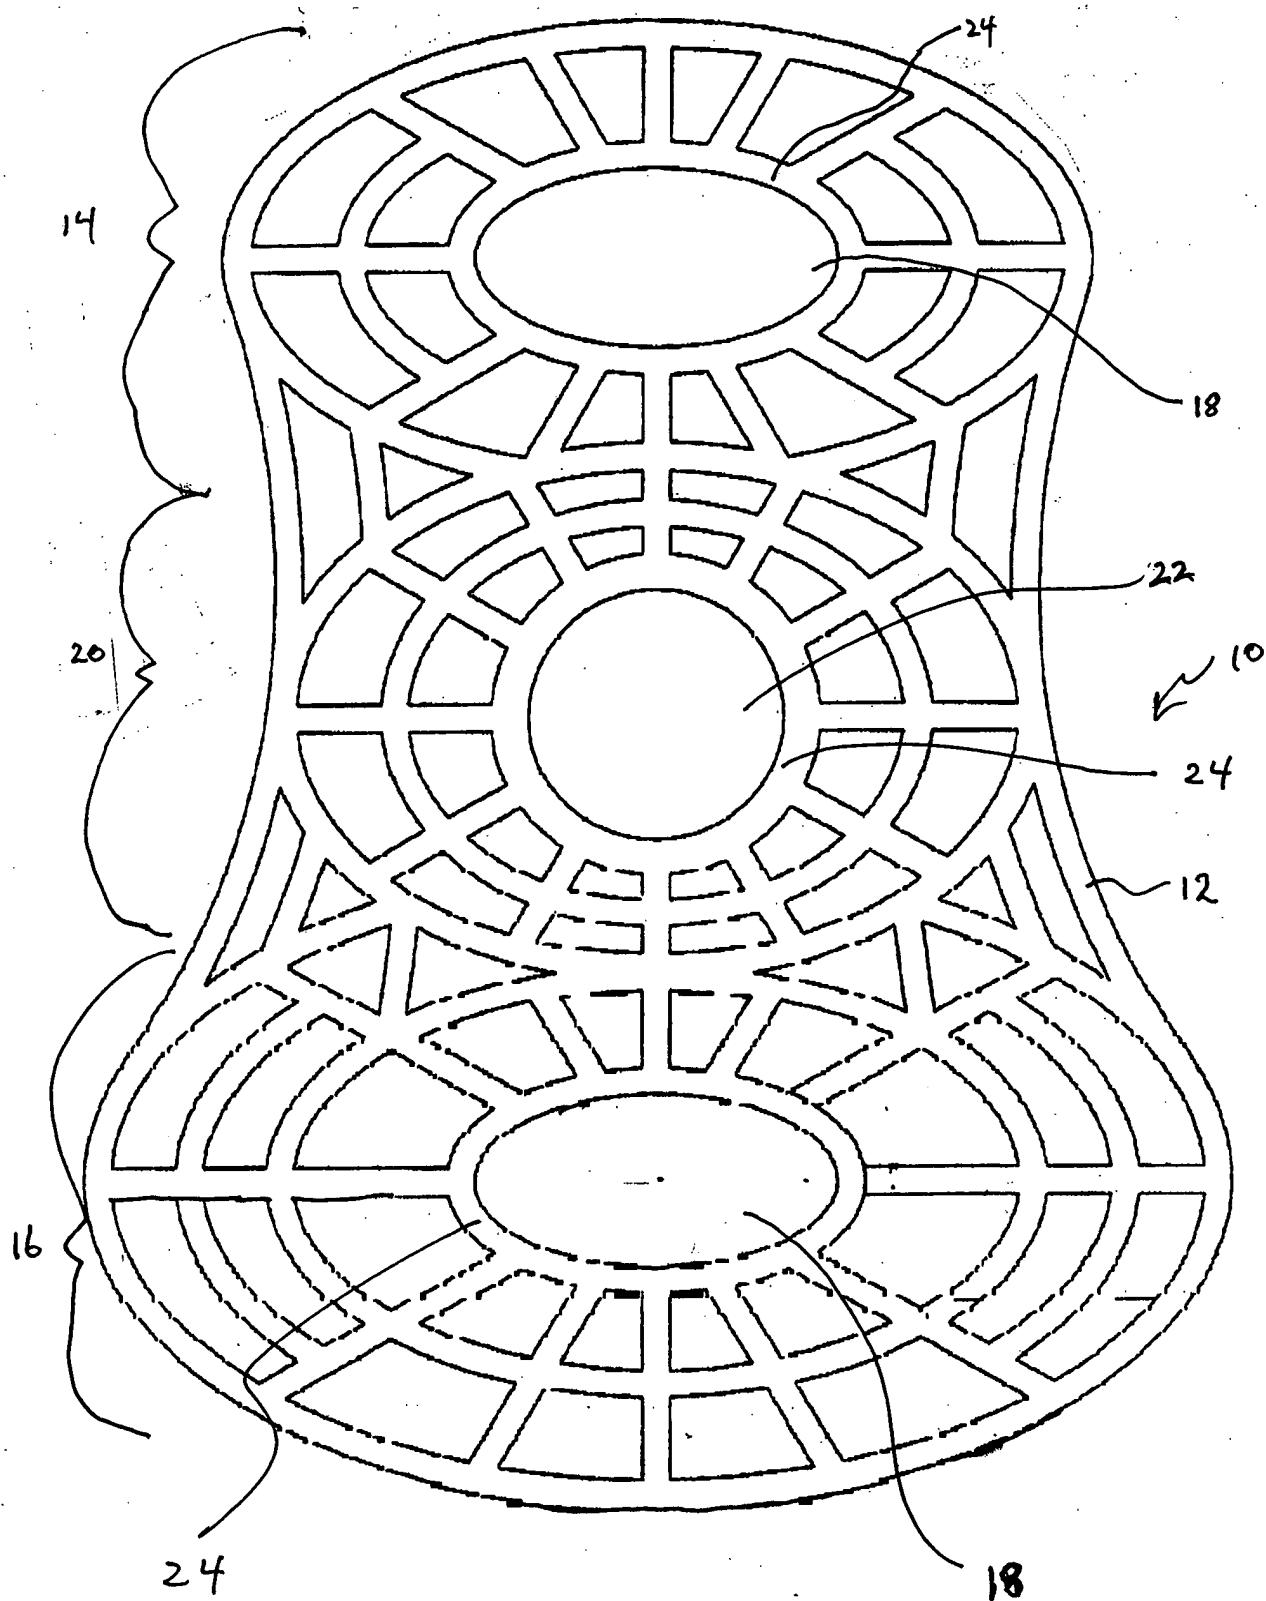


FIG. 1

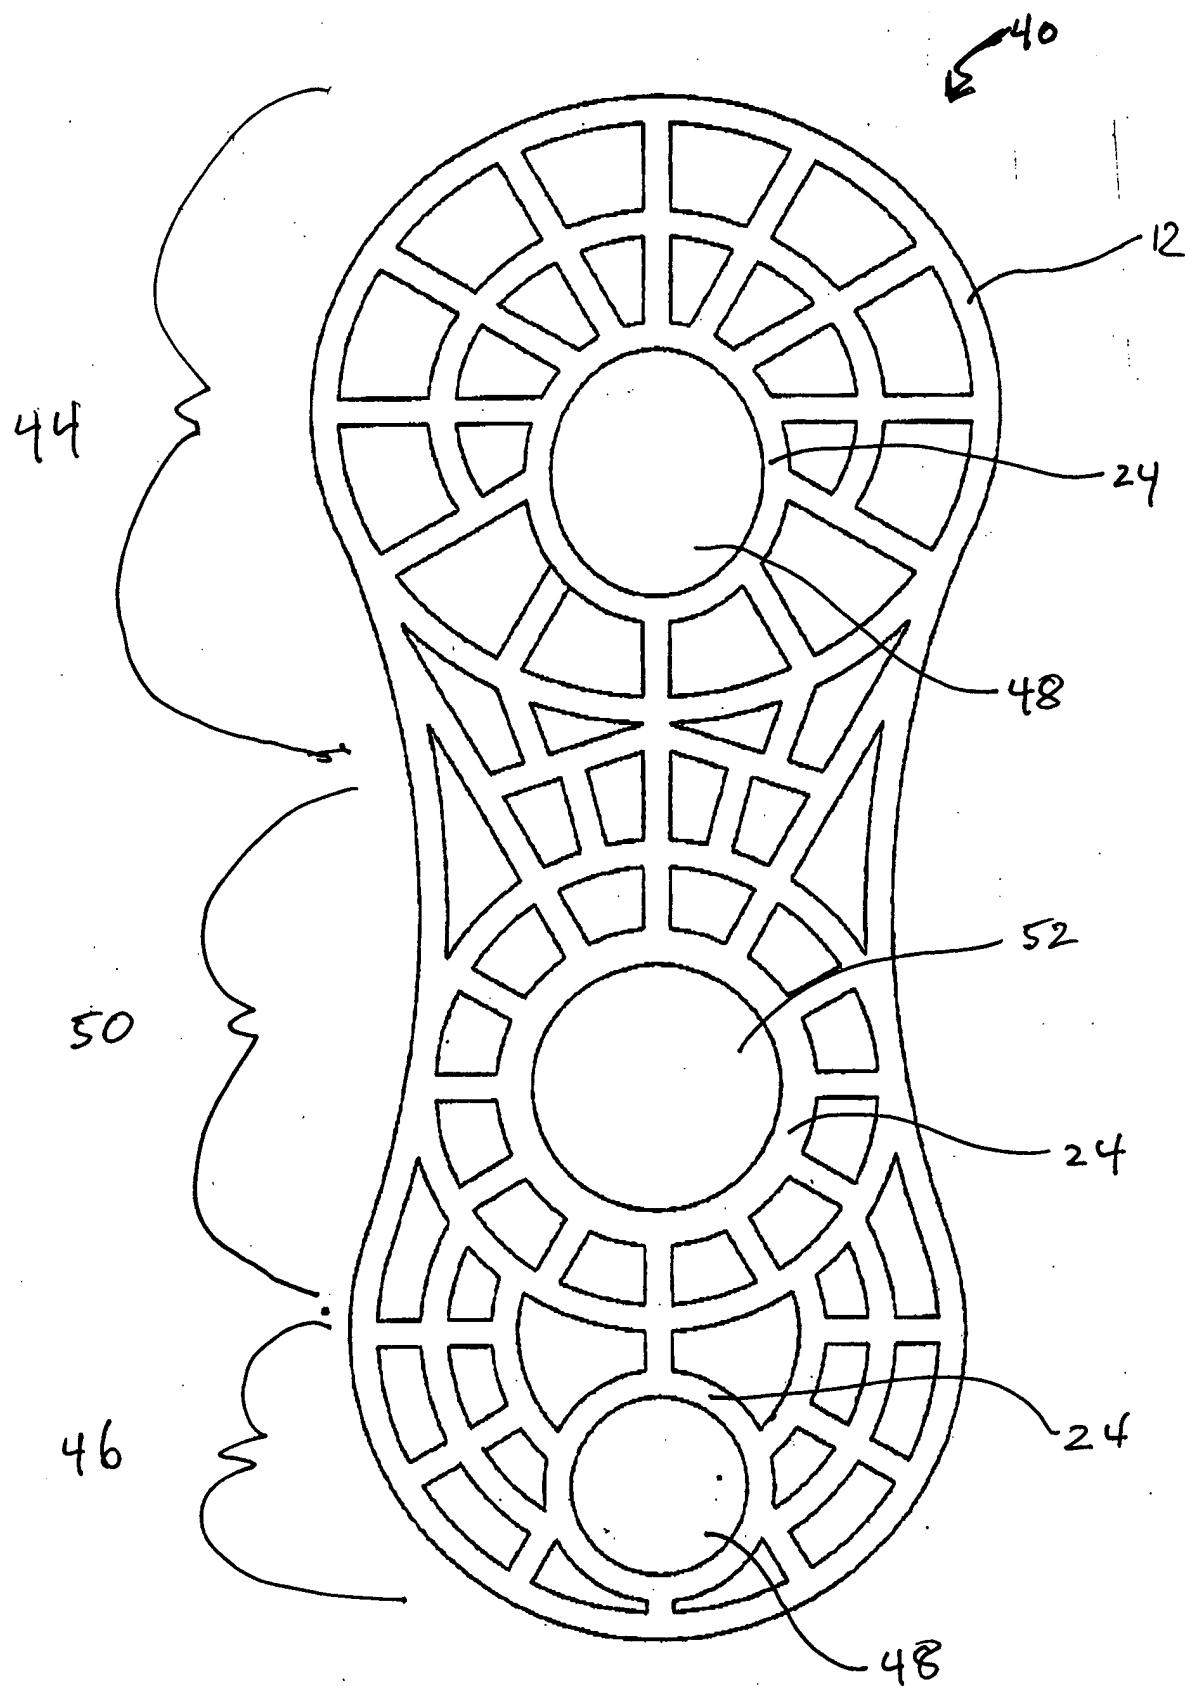


FIG. 2

Title: DEVICE FOR USE IN STIMULATING BONE GROWTH  
Applicant: Dane Q. Robinson, D.D.S.  
Docket No.: 26927.00015 Express Mail No. EV 229897298 US







Fig.  
3B              Fig.  
          3A

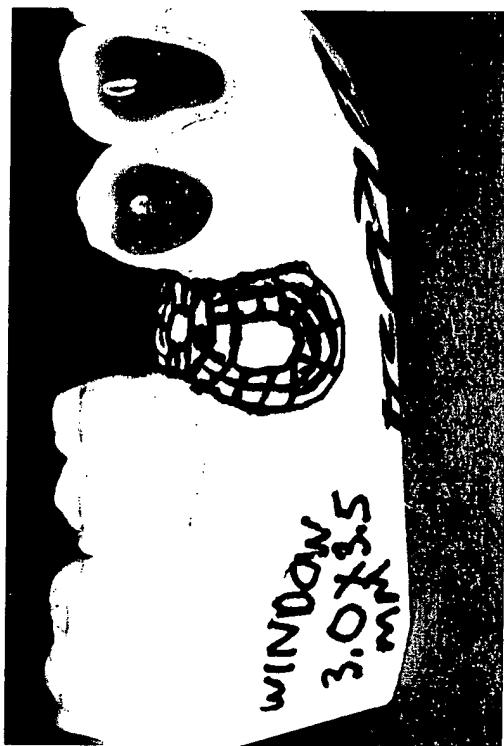

4B

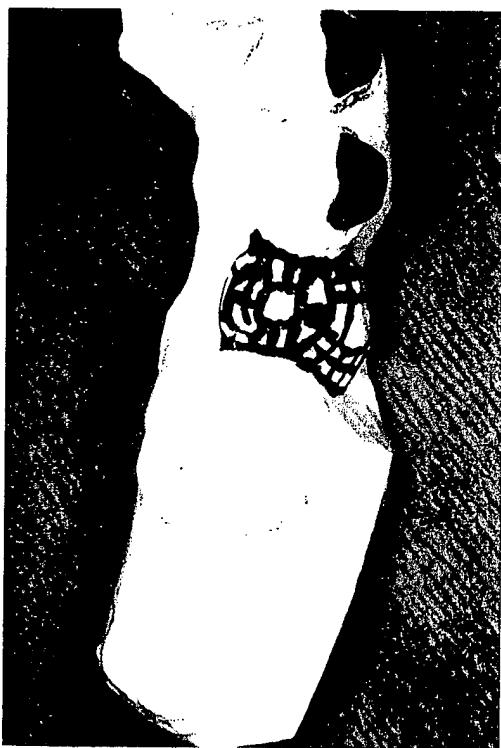


4A

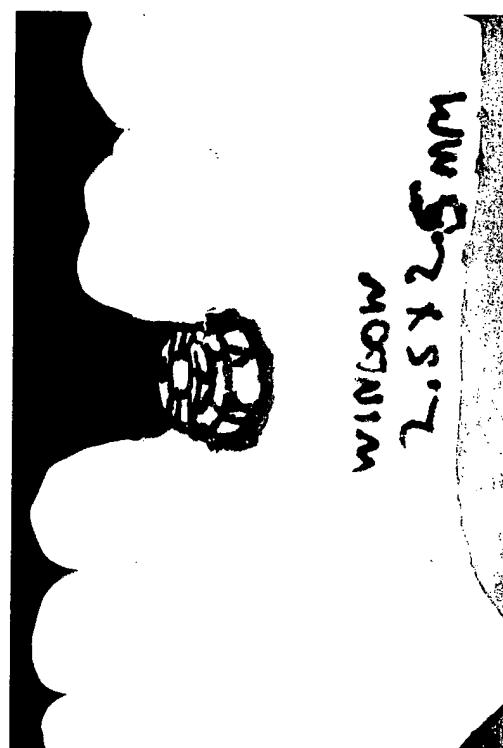


4C


Figs 4A-4C

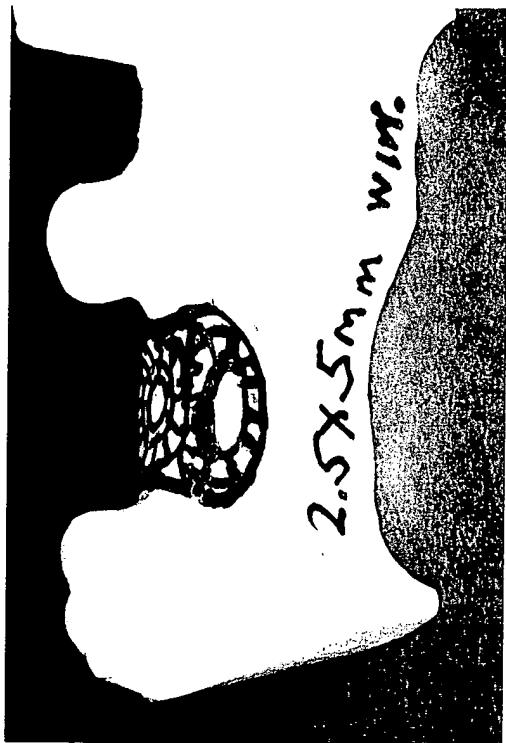

4D - 4F

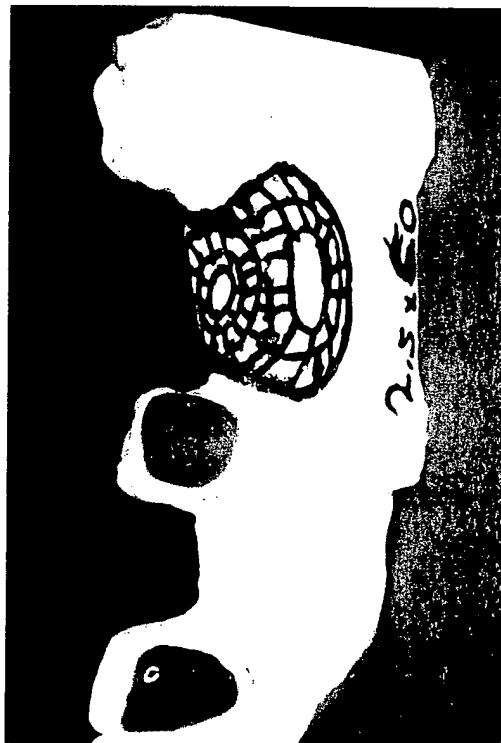

4D

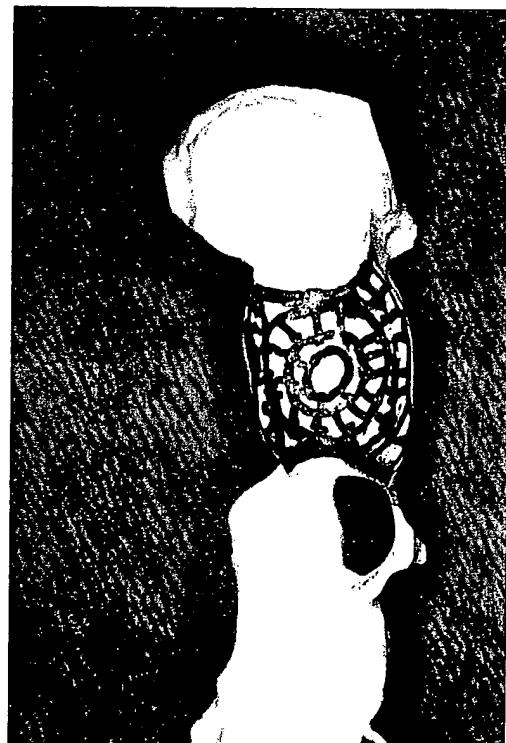

4F

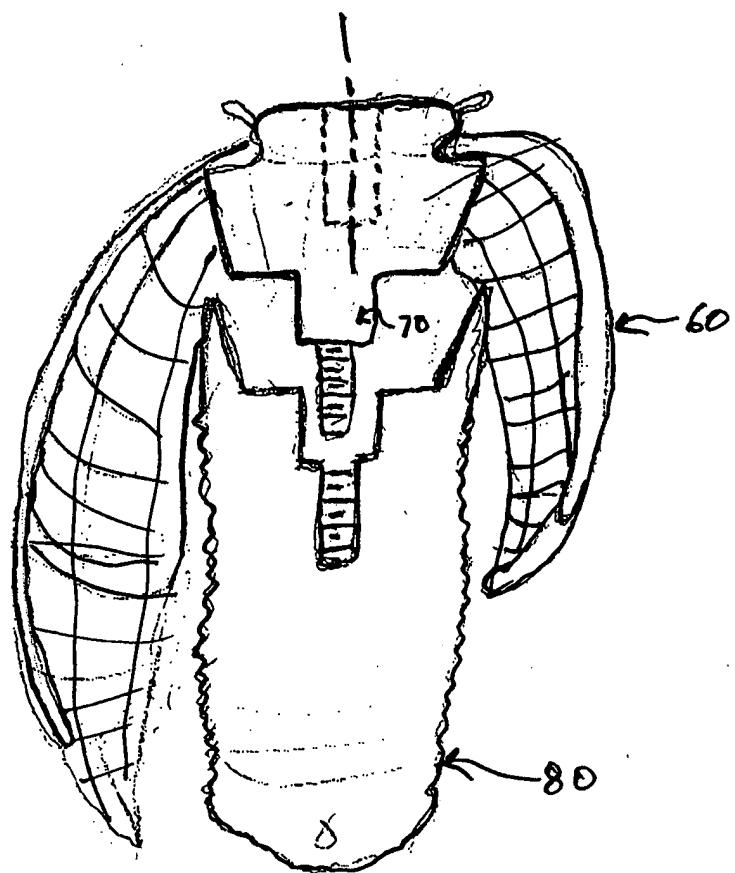


Fig. 5




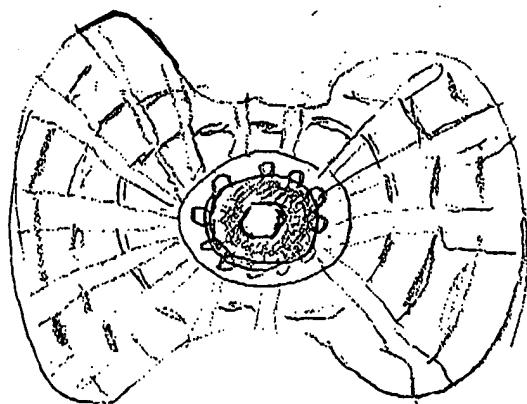


Fig. 6

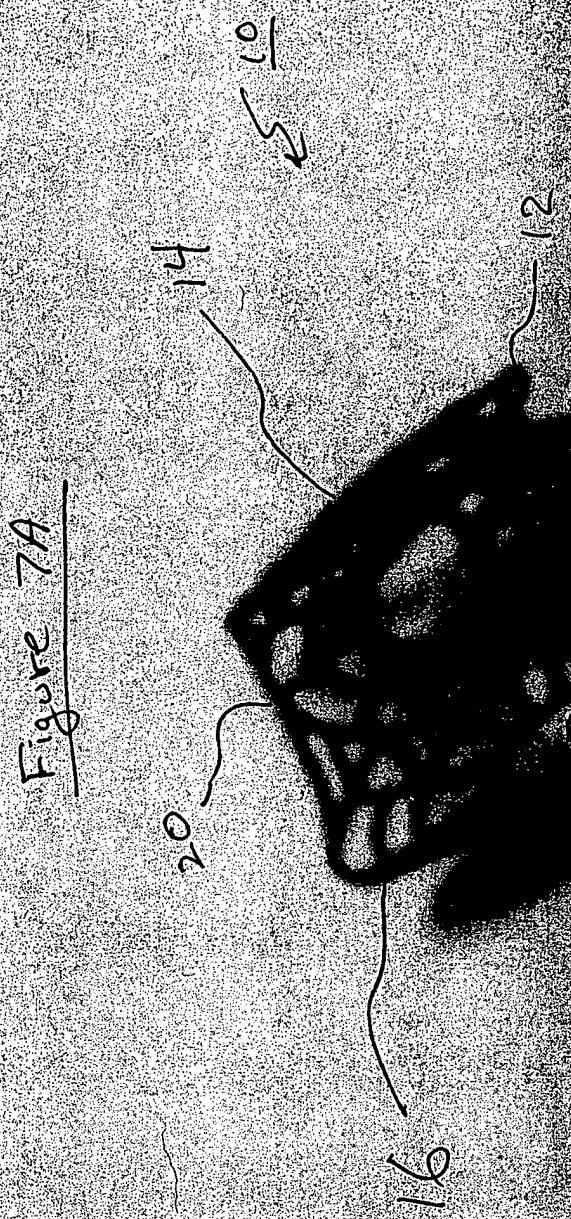

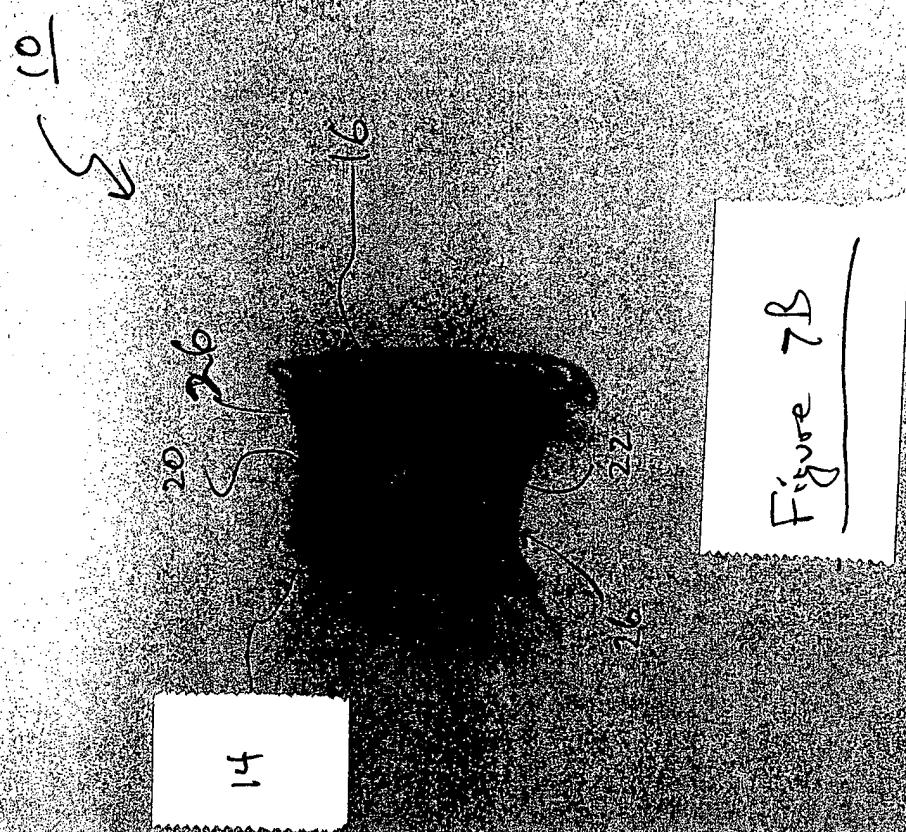

Title: DEVICE FOR USE IN STIMULATING BONE GROWTH  
Applicant: Dane Q. Robinson, D.D.S.  
Docket No.: 26927.00015 Express Mail No. EV 229897298 US

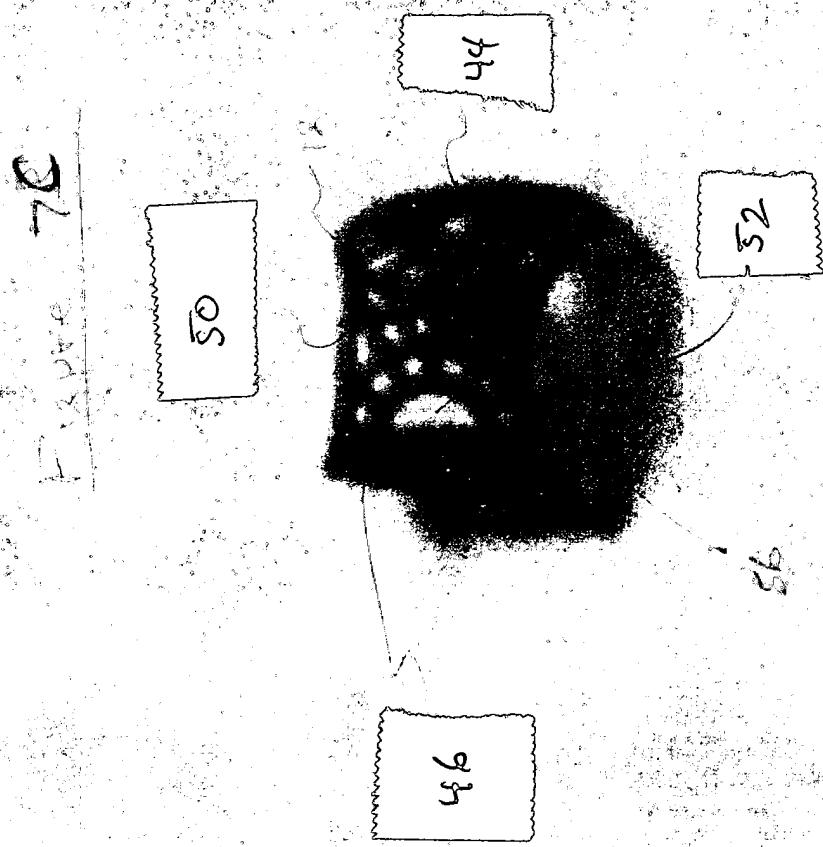



Title: DEVICE FOR USE IN STIMULATING BONE GROWTH  
Applicant: Dane Q. Robinson, D.D.S.  
Docket No.: 26927.00015 Express Mail No. EV 229897298 US

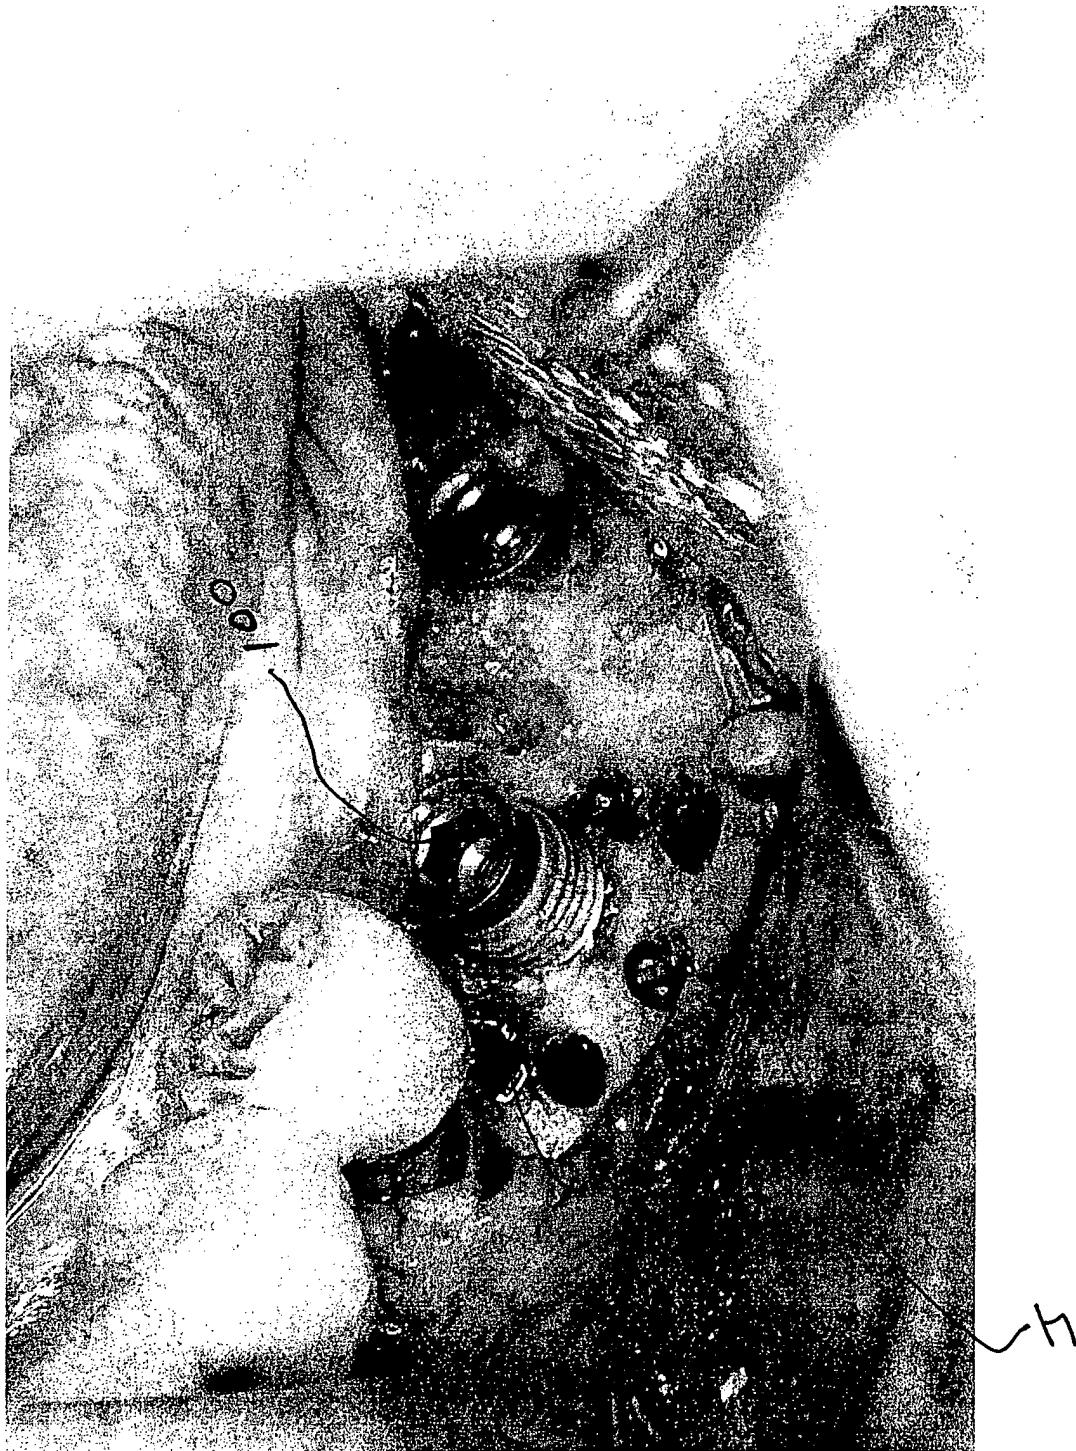


FIG. 8

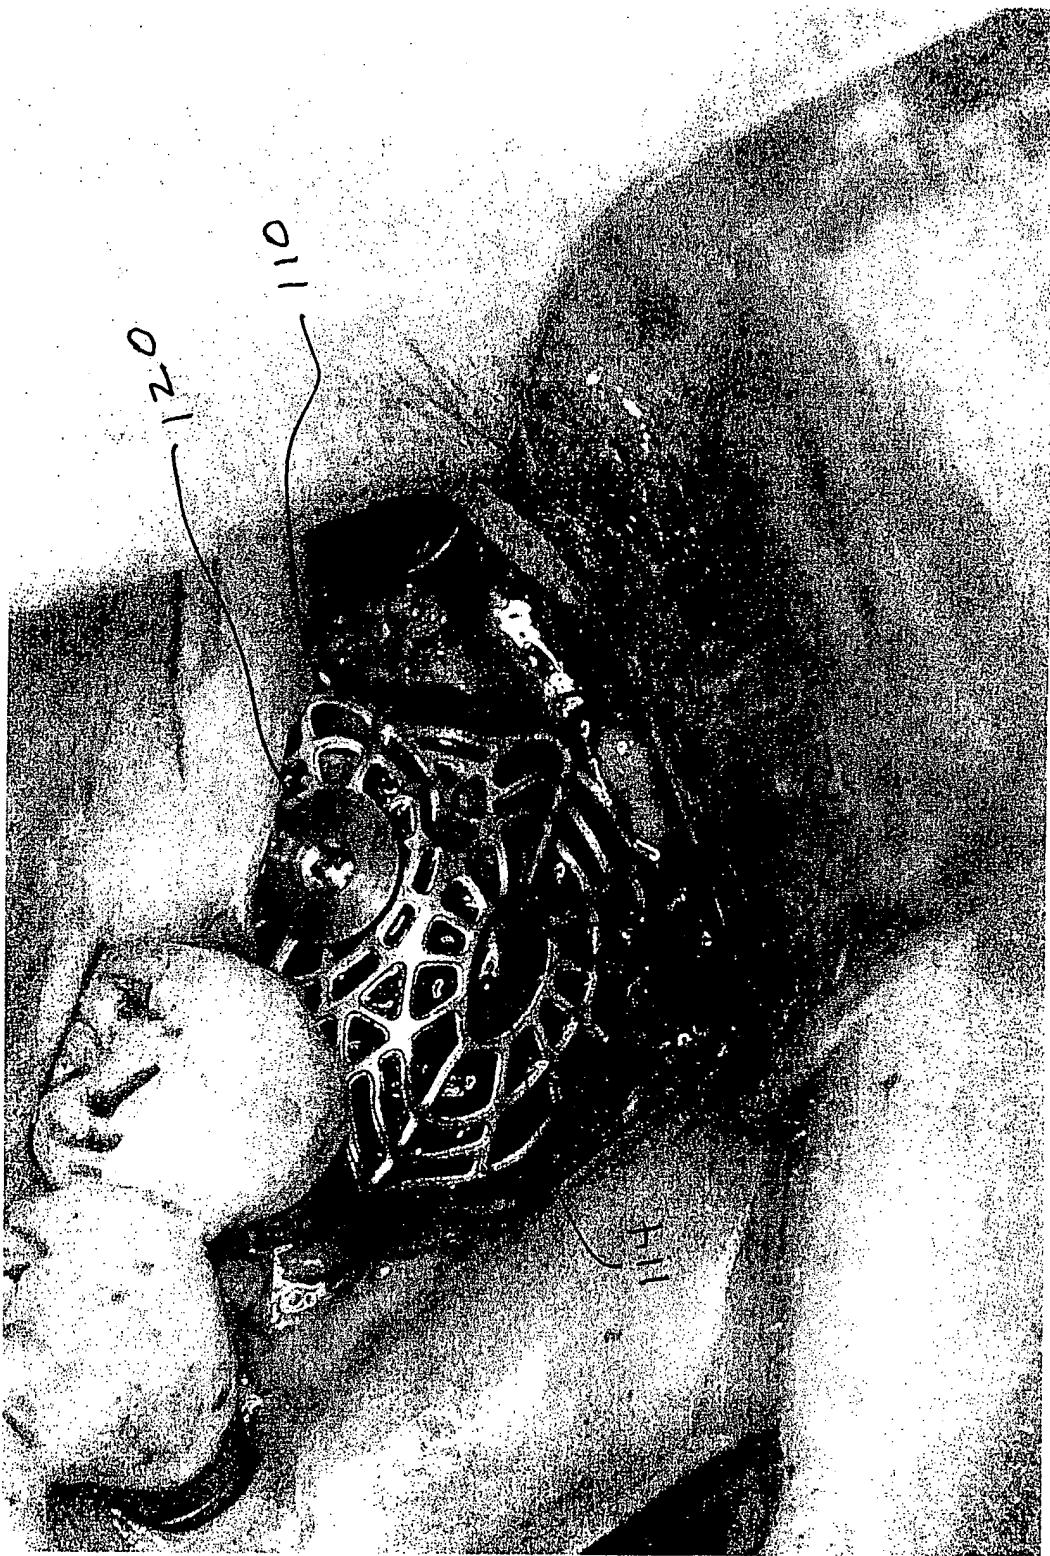


FIG. 9

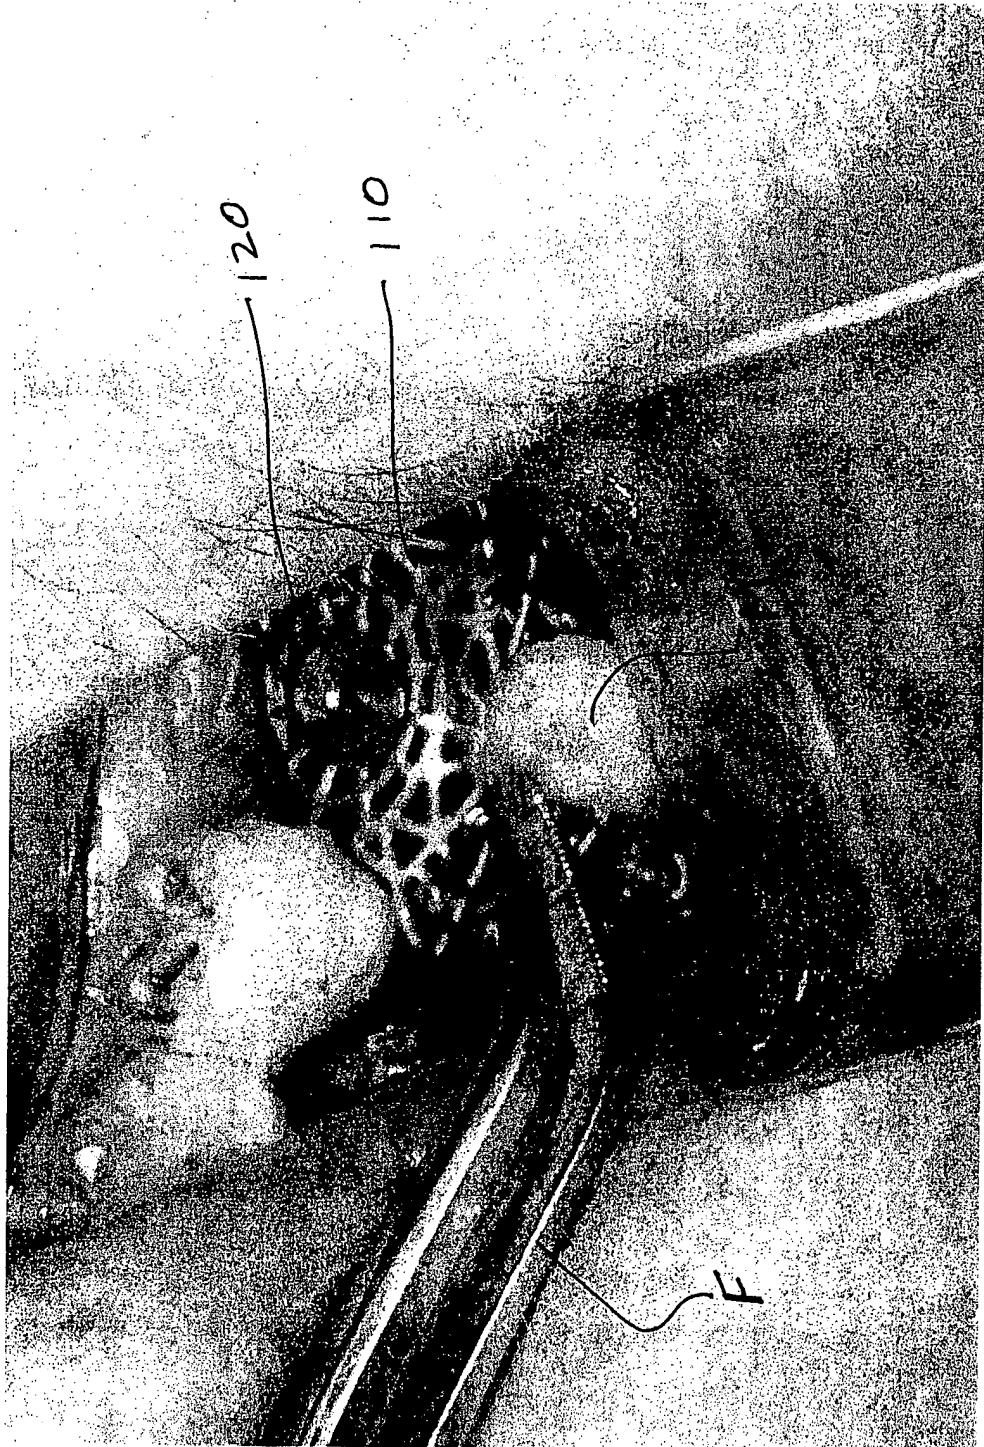


FIG. 10